


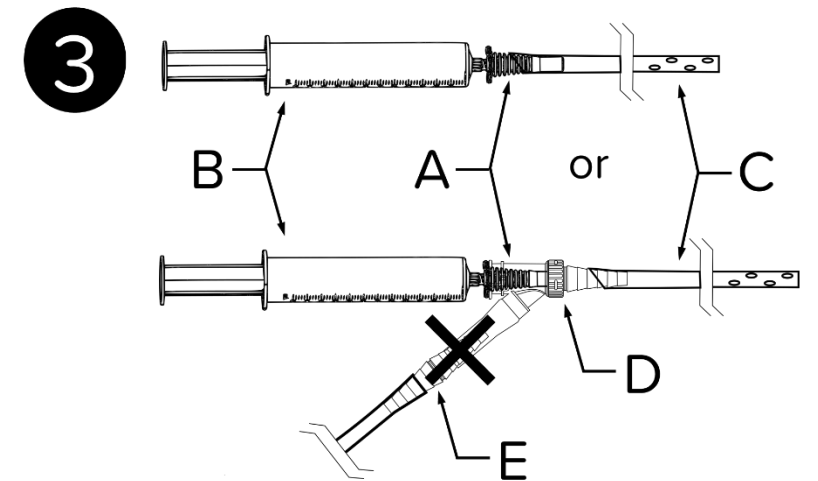
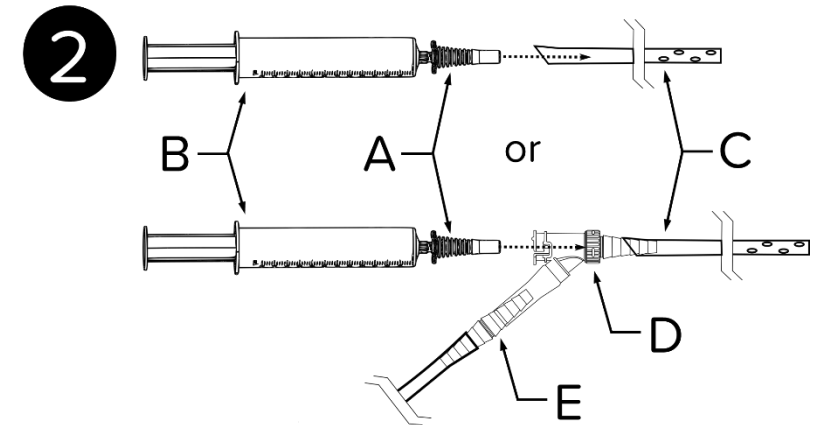
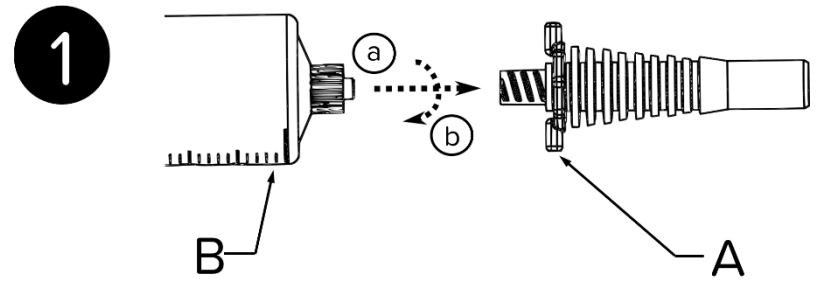


	EN ES FR IT 英语	Not made with natural rubber latex No fabricado con látex de caucho natural. Non fabriqué avec du latex de caoutchouc naturel Non realizzato con lattice di gomma naturale 不是用天然橡膠乳膠製成的
	EN ES FR IT 英语	Do not re-sterilize No volver a esterilizar Ne pas re-stériliser Non risterilizzare 不得重新消毒
	EN ES FR IT 英语	Expiration date Fecha de vencimiento date d'expiration Da utilizzare entro il 有效期
LOT	EN ES FR IT 英语	Lot number Número de lote Numéro de lot Codice partita 批号
DEHP FREE	EN ES FR IT 英语	DEHP free Sin DEHP sans DEHP Privo di DEHP 不含DEHP
	EN ES FR IT 英语	Caution Cuidado Attention Cautela 慎重
	EN ES FR IT 英语	Single patient use only Para uso exclusivo de un sólo paciente À l'usage exclusif d'un seul patient Monouso 限于单个病人使用
STERILE R	EN ES FR IT 英语	Sterilized by irradiation Esterilizado por irradiación Stérilisé par irradiation Sterilizzato con radiazione 放射消毒
Rx Only	EN ES FR IT 英语	Authorized for sale or use by physician only Autorizado para la venta o para el uso sólo por parte de un medico Autorisé à la vente ou à l'usage exclusif d'un médecin Autorizzato solo per vendita o uso da personale medico 医生授权后才可销售或使用
	EN ES FR IT 英语	See instructions for use Consultar las instrucciones de uso Consultez le mode d'emploi Vedere le istruzioni per l'uso 参见使用说明书
	EN ES FR IT 英语	Do not use if package is damaged No usar si el envoltorio está dañado Ne pas utiliser si l'emballage est endommagé Non utilizzare se l'imballaggio è danneggiato 包装损坏后不得使用
	EN ES FR IT 英语	Manufacture date Fecha de fabricación Date de fabrication Data di produzione 生产日期
Manufactured for: CLR® Medical Inc. 3901 Calverton Blvd, Suite 155 Calverton, MD 20705 USA TEL: 1-240-720-0673		www.CLRMedical.com

CLR® Port Injector – Instructions for use



⚠ BEFORE USING THIS PRODUCT, READ THE FOLLOWING INFORMATION THOROUGHLY**IMPORTANT!**

- These instructions are designed to assist with using this product. They should not be used as a guide for the performance of specific surgical techniques.
- This device was designed, tested and manufactured for single use only.
- Reuse of this device may lead to its failure and subsequent patient injury.
- Reprocessing and/or resterilization of this device may create risk of contamination and patient infection and lead to device failure.
- DO NOT reuse, reprocess or resterilize this device.

DESCRIPTION

The CLR® Port Injector is a catheter adapter configured for connecting male Luer syringes or infusion tubing to indwelling catheters directly or via the CLR Port.

INDICATIONS FOR USE

The CLR® Port Injector is intended to allow sampling or infusion through indwelling catheters.

CONTRAINDICATIONS

- This device is not intended for use except as indicated.

WARNINGS AND PRECAUTIONS

- Procedures should be performed only by medical providers who are trained in surgical techniques and failure modes, precautions, and corrective actions in the event of failure.
- This device is provided STERILE and is intended for SINGLE USE ONLY. DISCARD AFTER USE. DO NOT RESTERILIZE.
- Do not use product if the packaging sterile barrier is damaged.
- The CLR® Port Injector is DEHP free, not made with natural rubber latex, and is sterilized using gamma sterilization, except as noted.
- Dispose of all used or damaged products using standard hospital practices for biohazard control.

INSTRUCTIONS FOR USE

Inspect all components carefully for any damage that may have occurred during shipment, or where applicable, routine handling. Inspect packaging marked as sterile and verify that sterile barriers are intact. Do not use if sterile package is damaged or opened.

Follow the steps below for use of the CLR® Port Injector, referring to numbered images on Page 1.

Relevant Components

- A. CLR Port Injector
- B. Male Luer Syringe (or Infusion Tubing)
- C. Indwelling Catheter
- D. CLR Port
- E. Drainage System Collection Tubing

- 1** Attach Male Luer Syringe (or Infusion Tubing) to Port Injector
 - a. Insert male Luer adapter fitting into female Luer adapter fitting on Port Injector
 - b. Twist clockwise to thread the male Luer adapter fitting onto the Port Injector
- 2** Insert nozzle of Port Injector into Indwelling Catheter or CLR Port
- 3** Begin sampling or infusion by activating plunger of Syringe or unclamping Infusion Tubing. Note that if using CLR Port, the Drainage Collection System Tubing will be cut-off when the Port Injector is inserted to allow for direct infusion/sampling via the Indwelling Catheter.